Tech Service Products

1110 S. FM 1788 #42
Phone: (432) 296-4992 Email: Chad@tspndt.com
Midland,TX 79706

Certificate of Calibration

Certificate No TSPW-11022026-001

Gage ID	PEA-SDD175
Gage S/N	SDD175
Description	Lead Gauge
Operating Procedure:	OP-124
Unit of Meas.	Inch
Manufacturer	Gagemaker
Cal. Date	11/2/2026
Next Due	5/2/2027
Cal. Freq.	6.00 Months
Location	Lab

Environmental Conditions

Temperature	68 Deg F +/- 2
Humidity	20-55%

Approved	Yes
Customer Info.	Peak NDT Solutions

Certification Statement

TSP Calibration, Inc. calibration systems complies with the requirements of ISO 9001:2015. The equipment that is certified by this certificate has been calibrated by standards that have accuracy which is traceable to standards of the National Institute of Standards and Technology.

Findings

Order No. 1067815 Job No. 15317

As Found: Passed As Left: Passed

Contact Point Spacing at 1"
Target: 0.0040 Actual: 0.0040 Deviation: 0.0000

Contact Point Spacing at 2"
Target: 0.0080 Actual: 0.0080 Deviation: 0.0000

APPROVED
By Kayla Myers at 10:09 pm, Nov 03, 2026

Resolution: 0.0005" Tolerance: +/- 0.0010"

We certify the equipment used for this calibration is traceable to NIST through the following number(s):
Reference Standard: LS1007 Lead Gauge Standard - Serial Number: RG27AN0014
NIST Number: 314816 - Calibration Due Date: 1/27/2027

Reference Standard: LS1008 Lead Gauge Standard - Serial Number: HM25JK0010
NIST Number: 180668 - Calibration Due Date: 3/20/2027

Calibrated By Chad Adams **Signature** 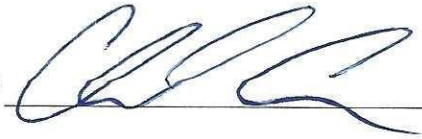 **Date:** 11/2/2026