

TSP Calibration, Inc.

1110 S. FM 1788 #42
 Phone: (432) 296-4992 Email: Chad@tspndt.com
 Midland, TX 79706

Certificate of Calibration

Certificate No TSPW-01162026-007

<p>Gage ID PEA-SKF112 Gage S/N SKF112 Description Lead Gauge Operating Procedure: OP-124 Unit of Meas. inch Manufacturer Gagemaker Cal. Date 1/16/2026 Next Due 7/16/2026 Cal. Freq. 6.00 Months Location Lab</p>	<p>Environmental Conditions Temperature 68 Deg F +/- 2 Humidity 35-55%</p> <p style="text-align: center;">Approved Yes Customer Info. Peak NDT Solutions</p>
--	--

Certification Statement

TSP Calibration, Inc. calibration systems complies with the requirements of ISO 9001:2015. The equipment that is certified by this certificate has been calibrated by standards that have accuracy which is traceable to standards of the National Institute of Standards and Technology.

Findings

SO 15392 Job 15125

As Found: Passed As Left: Passed

Contact point spacing at 1"
 Target 0.0040
 Actual 0.0040

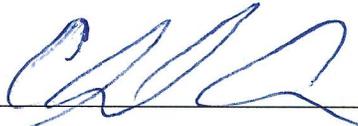
Contact point spacing at 2"
 Target 0.0080
 Actual 0.0080

Tolerance: +/- .0020"

APPROVED
 By Kayla Myers at 11:07 am, Jan 20, 2026

We certify the equipment used for this calibration is traceable to NIST through the following number(s):
 Reference Standard: LS1007 Lead Gauge Standard - Serial Number: JU06FM0027
 NIST Number: Doc#301641 - Calibration Due Date: 6/17/26

Reference Standard: LS1008 Lead Gauge Standard - Serial Number: RG15DM0010
 NIST Number: Doc#297680 - Calibration Due Date: 6/17/26

Calibrated By Chad Adams Signature  Date: 1/16/2026