

## TSP Calibration, Inc.

1110 S. FM 1788 Suite 38 Midland, TX 79706  
 Phone: (432) 296-4992 Email: Chad@tspndt.com

## Certificate of Calibration

Certificate No TSPW-07082025-016

<b>Gage ID</b> PEA-8235-1	<b>Environmental Conditions</b>  Temperature 68 Deg F +/- 2 Humidity 35-55%  <b>Approved</b> Yes <b>Customer Info.</b> Peak NDT Solutions
<b>Gage S/N</b> 8235-1	
<b>Description</b> 50-0-50 gauss meter	
<b>Operating Procedure:</b> OP-117	
<b>Unit of Meas.</b> gauss	
<b>Manufacturer</b> R.B. Annis	
<b>Cal. Date</b> 7/8/2025	
<b>Next Due</b> 1/8/2026	
<b>Cal. Freq.</b> 6.00 Months	
<b>Location</b> Lab	

## Certification Statement

TSP Calibration, Inc. calibration systems complies with the requirements of ISO 9001:2015. The equipment that is certified by this certificate has been calibrated by standards that have accuracy which is traceable to standards of the National Institute of Standards and Technology.

## Findings

SO 14534 Job 14212

<b>Standard ID</b> +25	<b>Uncertainty</b>	<b>Units</b>	<b>Type</b> V
<b>Limited Use?</b> No	<b>Minimum</b> 24	<b>Nominal</b> 25	<b>Maximum</b> 26
<b>Ref Type</b> 50-0-50 Gauss Meter	<b>As Found</b> 25	<b>Accuracy</b> 0	<b>Fail Before</b> No
	<b>As Left</b> 25	<b>Accuracy</b> 0	<b>Fail After</b> No
<b>Gage ID of Standard</b> REF-TSPSTD-01			
<b>Std Due Date</b> 8/8/2025	<b>Gage S/N</b> TSPSTD-01	<b>NIST No.</b> 154783	
<b>Standard ID</b> +50	<b>Uncertainty</b>	<b>Units</b>	<b>Type</b> V
<b>Limited Use?</b> No	<b>Minimum</b> 49	<b>Nominal</b> 50	<b>Maximum</b> 51
<b>Ref Type</b> 50-0-50 Gauss Meter	<b>As Found</b> 50	<b>Accuracy</b> 0	<b>Fail Before</b> No
	<b>As Left</b> 50	<b>Accuracy</b> 0	<b>Fail After</b> No
<b>Gage ID of Standard</b> REF-TSPSTD-01			
<b>Std Due Date</b> 8/8/2025	<b>Gage S/N</b> TSPSTD-01	<b>NIST No.</b> 154783	
<b>Standard ID</b> -25	<b>Uncertainty</b>	<b>Units</b>	<b>Type</b> V
<b>Limited Use?</b> No	<b>Minimum</b> 24	<b>Nominal</b> 25	<b>Maximum</b> 26

Ref Type	50-0-50 Gauss Meter	As Found	25	Accuracy	0	Fail Before	No
		As Left	25	Accuracy	0	Fail After	No

Gage ID of Standard REF-TSPSTD-01

Std Due Date 8/8/2025

Gage S/N TSPSTD-01 NIST No. 154783

Standard ID	-50	Uncertainty		Units		Type	V
Limited Use?	No	Minimum	49	Nominal	50	Maximum	51
Ref Type	50-0-50 Gauss Meter	As Found	50	Accuracy	0	Fail Before	No
		As Left	50	Accuracy	0	Fail After	No


Gage ID of Standard REF-TSPSTD-01

Std Due Date 8/8/2025

Gage S/N TSPSTD-01 NIST No. 154783

Calibrated By Chad Adams

Signature

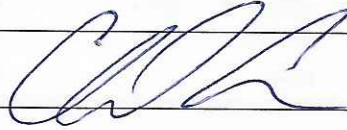

Date: 7/8/2025

**APPROVED***By Kayla Myers at 8:41 am, Aug 15, 2025*