

## TSP Calibration, Inc.

1110 S. FM 1788 Suite 38 Midland, TX 79706  
Phone: (432) 296-4992 Email: Chad@tspndt.com

## Certificate of Calibration

Certificate No TSPW-02132025-010

|   |   |
|---|---|
| <b>Gage ID</b> PEA-2419001777<br><b>Gage S/N</b> 2419001777<br><b>Description</b> UV Light Meter<br><b>Operating Procedure:</b> OP-119<br><b>Unit of Meas.</b> Microwatts/cm2<br><b>Manufacturer</b> General<br><b>Cal. Date</b> 2/13/2025<br><b>Next Due</b> 8/13/2025<br><b>Cal. Freq.</b> 6.00 Months<br><b>Location</b> Lab | <b>Environmental Conditions</b><br><b>Temperature</b> 68 Deg F +/- 2<br><b>Humidity</b> 35-55%<br><br><b>Approved</b> Yes<br><b>Customer Info.</b> Peak NDT Solutions |
|---|---|

## Certification Statement

TSP Calibration, Inc. calibration systems complies with the requirements of ISO 9001:2015. The equipment that is certified by this certificate has been calibrated by standards that have accuracy which is traceable to standards of the National Institute of Standards and Technology.

## Findings


Calibrated black light serial no. 1911981 was used during this calibration.  
Calibration due date for black light is on 8/8/2025  
Black light is traceable to NIST by the following numbers: Doc# 154779

|                     |             |             |         |          |        |             |        |
|---------------------|-------------|-------------|---------|----------|--------|-------------|--------|
| Standard ID         | 12"         | Uncertainty |         | Units    |        | Type        | V      |
| Limited Use?        | No          | Minimum     | 2891.8  | Nominal  | 3044   | Maximum     | 3196.2 |
| Ref Type            | Light Meter | As Found    |         | Accuracy |        | Fail Before | No     |
|                     |             | As Left     |         | Accuracy |        | Fail After  | No     |
| Gage ID of Standard | REF-1705427 |             |         |          |        |             |        |
| Std Due Date        | 8/12/2025   | Gage S/N    | 1705427 | NIST No. | 154789 |             |        |

|                     |             |             |         |          |        |             |         |
|---------------------|-------------|-------------|---------|----------|--------|-------------|---------|
| Standard ID         | 15"         | Uncertainty |         | Units    |        | Type        | V       |
| Limited Use?        | No          | Minimum     | 2014.95 | Nominal  | 2121   | Maximum     | 2227.05 |
| Ref Type            | Light Meter | As Found    |         | Accuracy |        | Fail Before | No      |
|                     |             | As Left     |         | Accuracy |        | Fail After  | No      |
| Gage ID of Standard | REF-1705427 |             |         |          |        |             |         |
| Std Due Date        | 8/12/2025   | Gage S/N    | 1705427 | NIST No. | 154789 |             |         |

Calibrated By Chad Adams

Signature

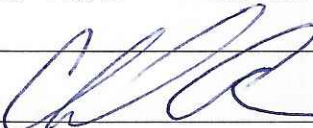

Date: 2/13/2025

**APPROVED**

*By Kayla Myers at 11:27 am, Mar 03, 2025*