

# TSP Calibration, Inc.

1110 S. FM 1788 #42  
 Phone: (432) 296-4992 Email: Chad@tspndt.com  
 Midland, TX 79706

## Certificate of Calibration

Certificate No TSPW-04062026-017

<p><b>Gage ID</b> PEA-1968110  <b>Gage S/N</b> 1968110  <b>Description</b> Dual Light Meter  <b>Operating Procedure:</b> OP-119/OP-130  <b>Unit of Meas.</b> Microwatts/cm2 &amp; Foot Candles  <b>Manufacturer</b> Spectroline  <b>Cal. Date</b> 4/6/2026  <b>Next Due</b> 10/6/2026  <b>Cal. Freq.</b> 6.00 Months  <b>Location</b> Lab</p>	<p><b>Environmental Conditions</b>                  Temperature 68 Deg F +/- 2                  Humidity 35-55%</p> <p style="text-align: center;"><b>Approved</b> Yes  <b>Customer Info.</b> Peak NDT Solutions</p>
---	--

**Certification Statement**

TSP Calibration, Inc. calibration systems complies with the requirements of ISO 9001:2015. The equipment that is certified by this certificate has been calibrated by standards that have accuracy which is traceable to standards of the National Institute of Standards and Technology.

**Findings**

Visible Light Readings:	Master	As Found	
High:	108.6	107.9	
Low:	19.4	18.6	

NOTE: IF ONLY AN "AS FOUND" READING IS STATED, "AS FOUND" AND "AS LEFT" READINGS ARE THE SAME WITH NO ADJUSTMENTS.

Tolerance: +/-5% or +/-2 foot candles, whichever is greater.

We certify the equipment used for this calibration is traceable to NIST through the following number(s):

Reference Standard: UV Light - Serial Number: 1911981  
 NIST Number: Doc#171852 - Calibration Due Date: 8/21/2026

Reference Standard: Dual Light Meter - Serial Number: 1705427 Sensor: 1705430  
 NIST Number: Doc#171854 - Calibration Due Date: 8/21/2026

UV Light Readings

Standard ID	12"	Uncertainty	Units	Type	V
Limited Use?	No	Minimum	2952.6	Nominal	3108
Ref Type	Light Meter	As Found	3141	Accuracy	33
		As Left	3141	Accuracy	33
Gage ID of Standard		REF-1705427			
Std Due Date		8/21/2026			
Gage S/N		1705427			
NIST No.		171854			

Standard ID	15"	Uncertainty		Units		Type	V
Limited Use?	No	Minimum	2150.8	Nominal	2264	Maximum	2377.2
Ref Type	Light Meter	As Found	2284	Accuracy	20	Fail Before	No
		As Left	2284	Accuracy	20	Fail After	No

Gage ID of Standard REF-1705427


Std Due Date 8/21/2026

Gage S/N 1705427

NIST No. 171854

Calibrated By Chad Adams

Signature

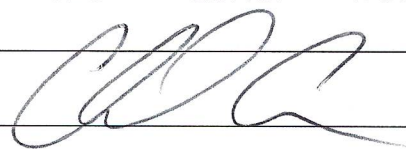

Date: 4/6/2026

**APPROVED**

*By Kayla Myers at 9:51 am, Apr 14, 2026*